

UHPLC CERTIFICATE OF ANALYSIS

SAMPLE INFORMATION

Sample received:

Product Name	Retatrutide Batch No. 12731
Sequence	Tyr-{Aib}-Gln-Gly-Thr-Phe-Thr-Ser-Asp-Tyr-Ser-Ile-{α-Me-Leu}-Leu-Asp-Lys-{diacid-C20-γ-Glu-(AEEA)-Lys}-Ala-Gln-{Aib}-Ala-Phe-Ile-Glu-Tyr-Leu-Leu-Glu-Gly-Gly-Pro-Ser-SerGly-Ala-Pro-Pro-Pro-Ser-NH ₂
Dissolution Condition	100% UHPLC water with 0.1% Trifluoroacetic Acid (TFA). Dissolved sample picture included here. 
Molecular Weight	~4,731.3 g·mol ⁻¹

STORAGE CONDITION: 0 °C

SAMPLE NOTES

One 3 ml clear glass vial with violet cap and silver aluminum crimp. Lyophilized powder present.



PUMP SETTINGS

Pump A	100% H2O with .1% Trifluoroacetic Acid
Pump D	100% Acetonitrile.
Column Usage	Agilent Zorbax 300SB-C18, 2.1 x 100 mm, 1.7 µm, 300 Å
Gradient	- 5% D hold (0–1 min) - 5–40% D over 18 min (1.9% D/min) - Hold 40% D (3 min) - Re-equilibrate to 5% D over 3 min - Total run time: ~25 min.
Pump Settings	0.6 mL/min
Injection Volume:	10 µL
Temperature	30 °C


PURITY RESULT

Purity is **99.52%**

Product weight extrapolation: 5.8mg

Total impurity 0.48% (trace inert solvents and minor unidentified peaks; no significant related substances or degradation products detected above 0.1%).

Chromatogram Export: please note that x axis represents elution window.

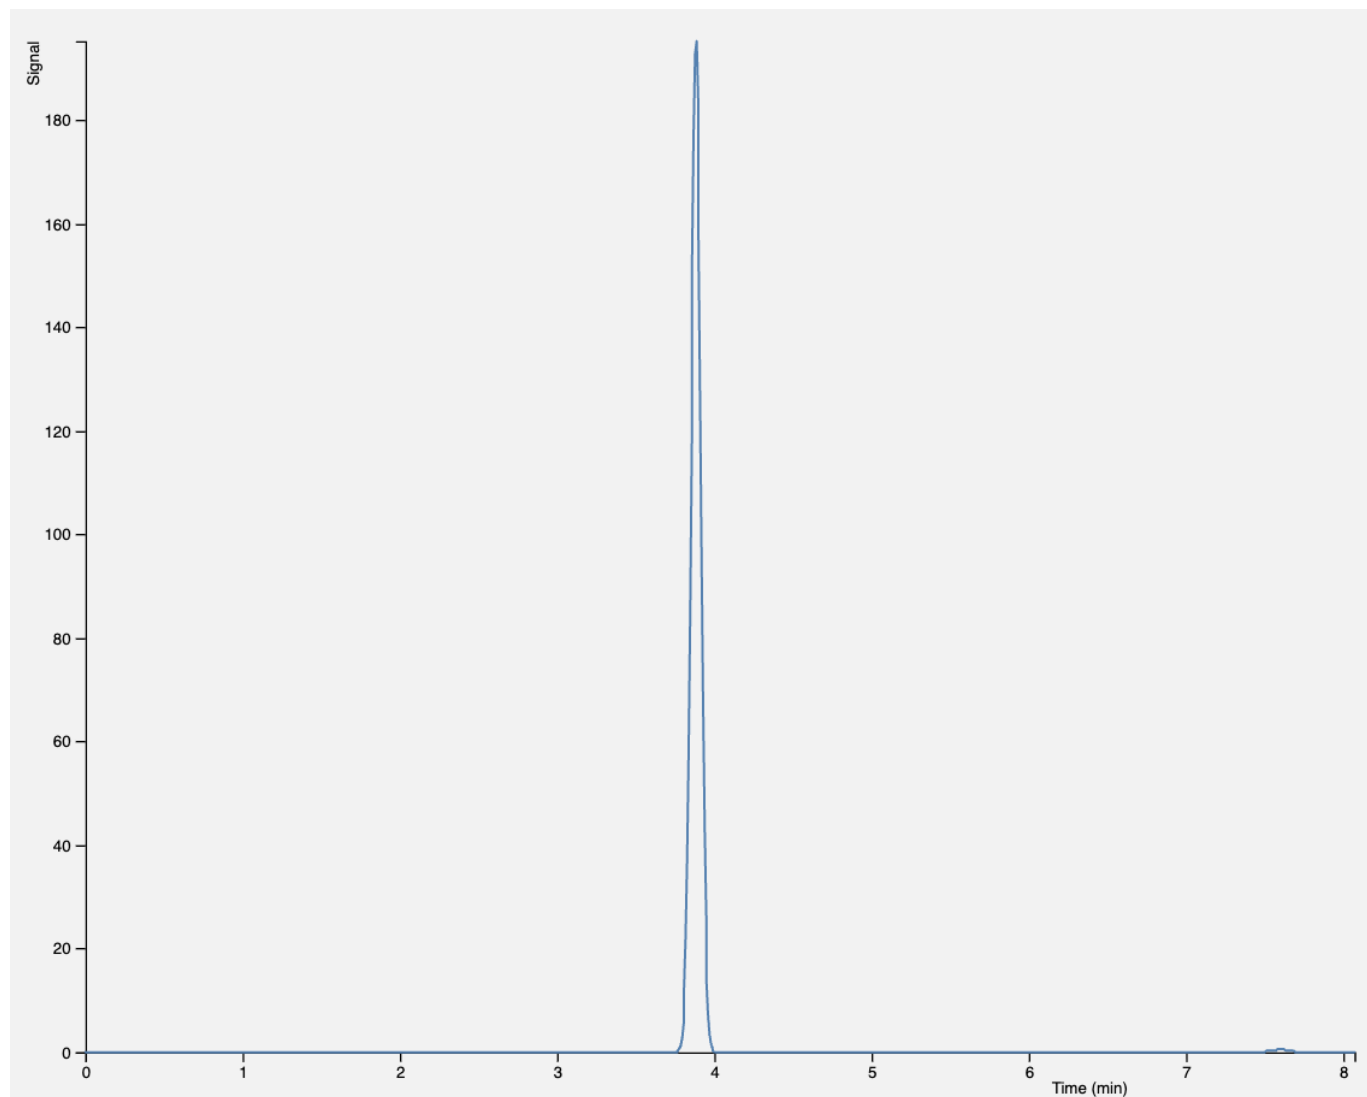

CONCLUSION

This sample was analyzed on a Thermo Ultimate U3000 HPLC stack using reverse-phase high-performance liquid chromatography and determined to contain **99.52% Retatrutide**, with the remainder being impurities of minor significance.

CERTIFICATION

Certified by: Jonathan Barber

Title: Analytical Chemist

Date: 10 September 2025



Trulab Peptides www.trulabpeptides.com | **Phone:** 872-239-6582

Address: 15017 North Dale Mabry Highway #1121 Tampa, FL 33618 United States