


UHPLC CERTIFICATE OF ANALYSIS

SAMPLE INFORMATION


Sample received:

Product Name	Selank 5mg Batch No. 73527
Sequence	Thr-Lys-Pro-Arg-Pro-Gly-Pro
Dissolution Condition	<p>100% UHPLC water with 0.1% Trifluoroacetic Acid (TFA). Dissolved sample picture included here.</p> 
Molecular Weight	~751.9 g/mol

STORAGE CONDITION: 0 °C

SAMPLE NOTES

One 3 ml clear glass vial with silver cap and silver aluminum crimp. Lyophilized powder present.

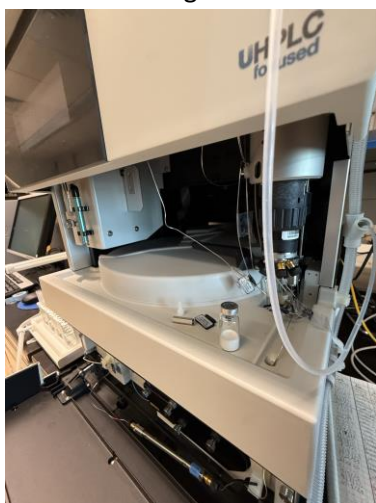

PUMP SETTINGS

Pump A	100% H2O with .1% Trifluoroacetic Acid
Pump D	100% Acetonitrile.
Column Usage	Agilent Zorbax 300SB-C18, 2.1 x 100 mm, 1.7 μ m, 300 Å
Gradient	- 5% D hold (0–0.5 min) - 5 \rightarrow 35% D over 8 min (\approx 3.75% D/min) - 35 \rightarrow 50% D over 3 min (flush more hydrophobic impurities) - Hold 50% D (2 min) - Re-equilibrate to 5% D over 3 min - Total run time: \sim 16.5 min.
Pump Settings	0.6 mL/min
Injection Volume:	10 μ L
Temperature	30 $^{\circ}$ C


PURITY RESULT

Purity is **99.44%**

Product weight extrapolation: 5.8mg

Total impurity 0.56% (trace inert solvents and minor unidentified peaks; no significant related substances or degradation products detected above 0.1%).

Chromatogram Export: please note that x axis represents elution window.

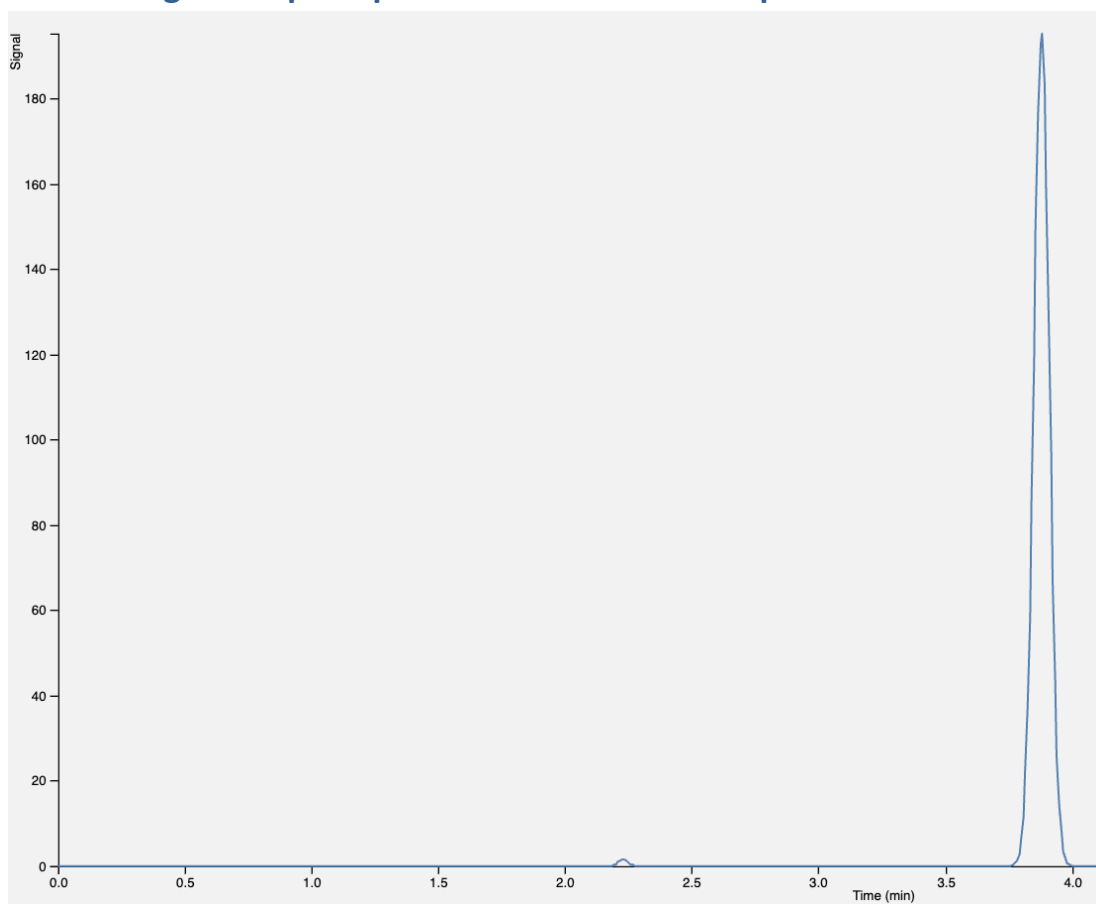

CONCLUSION

This sample was analyzed on a Thermo Ultimate U3000 HPLC stack using reverse-phase high-performance liquid chromatography and determined to contain **99.44% Selank** with the remainder being impurities of minor significance.

CERTIFICATION

Certified by: Jonathan Barber

Title: Analytical Chemist

Date: 13 December 2025



Trulab Peptides www.trulabpeptides.com | **Phone:** 872-239-6582
Address: 15017 North Dale Mabry Highway #1121 Tampa, FL 33618 United States